


REVISIONS				
ZONE	REV	DESCRIPTION	DATE	APPROVED


NOTES:
 THE ANALYZER SHOULD BE PIPED,
 WIRED AND GROUNDED IN ACCORDANCE
 WITH ALL LOCAL CODES AND ORDANCES.

ZFK2 OXYGEN DETECTOR




CONNECTING CABLE ZKM TO ZFK
 CONDUIT (INSTALLED BY CUSTOMER)
 CONNECTING CABLE LENGTHS UP TO
 1000 FT ARE AVAILABLE AS AN OPTION.

ZKM OXYGEN TRANSMITTER

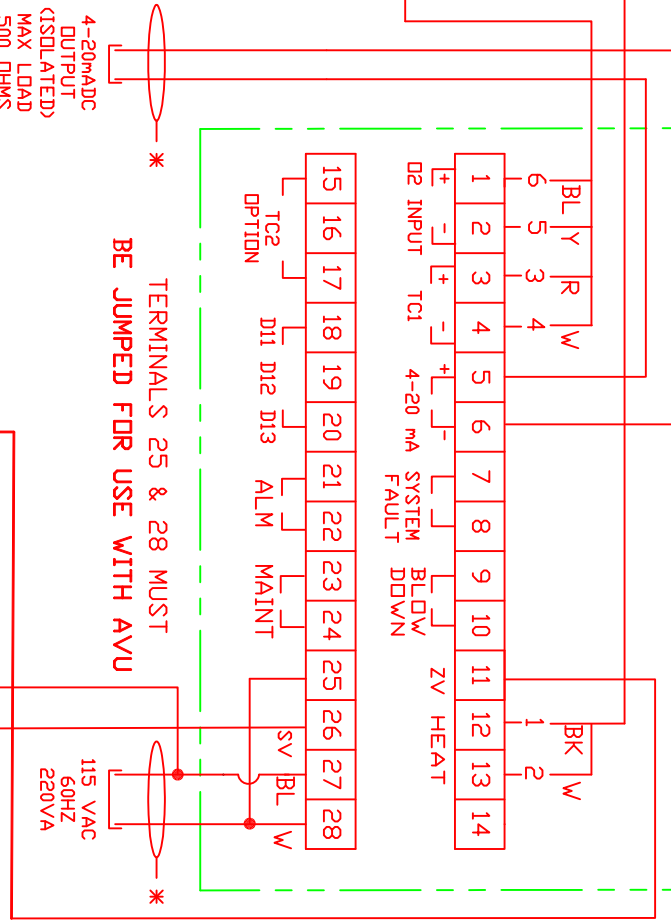

TERMINALS 25 & 28 MUST
 BE JUMPED FOR USE WITH AVU



Auto Verification Unit

Delta Instrument LLC		SCALE	
ZKM Auto Verification Unit Wiring		SIZE	FSQM NO.
		DWG NO.	REV
		SHEET	